



® Knowledge Beyond Measure.

Aerodynamic Particle Sizer®

Model 3321



High-resolution aerodynamic sizing plus light-scattering intensity

The Aerodynamic Particle Sizer® (APSTM) 3321 spectrometer provides high resolution, real-time aerodynamic measurements of particles from 0.5 to 20 μm . This unique particle sizer also measures light-scattering intensity in the equivalent optical size range of 0.37 to 20 μm . By providing paired data for each particle, the APSTM spectrometer opens up exciting new possibilities for those interested in studying the makeup of an aerosol.

The APSTM spectrometer uses a patented*, double-crest optical system for unmatched sizing accuracy. It also includes a redesigned nozzle configuration and improved signal processing. The result is greater small-particle sizing efficiency, improved accuracy of mass-weighted distributions, and virtual elimination of false background counts.

*US Patent # 5,561,515.

Features and Benefits

- Double-crest optics produce high-quality measurements
- Measures aerodynamic particle size from 0.5 to 20 μm
- Measures light-scattering intensity from 0.37 to 20 μm
- Real-time aerodynamic sizing
- No need to wait for cascade impactor measurements
- High size resolution – 52 size channels
- Independent of optical properties of the particles and fluid

Applications

- Inhalation toxicology
- Drug delivery studies
- Atmospheric studies
- Ambient air monitoring
- Indoor air quality monitoring
- Filter and air cleaner testing
- Biohazard detection
- Test aerosols characterization
- Usable for particle instrument calibration
- Spray technology
- Performance evaluations of aerodynamic devices
- Powder sizing
- Basic research

Why is Aerodynamic Diameter Important?

Aerodynamic diameter is defined as the physical diameter of a unit density sphere that settles through the air with a velocity equal to that of the particle in question. It is the most significant aerosol size parameter because it determines the particle's behavior while airborne. Particles exhibiting the same airborne behavior have the same aerodynamic diameter, regardless of their physical size, shape, density, or composition.


Knowledge of a particle's aerodynamic diameter allows you to determine:

- If and where the particle will be deposited in the human respiratory tract
- How long the particle will remain airborne in the atmosphere or in an aerosol
- Whether the particle will penetrate a filter, cyclone, or other particle-removing device
- Whether the particle will enter a particle-sampling system
- Whether the particle will penetrate a pipe, tube, duct, or channel

Why is the Model 3321 Superior?



Traditionally, TSI® has designed its time-of-flight spectrometers to provide the truest high-resolution measurements of aerodynamic size. With the introduction of the model 3320 in 1997, TSI produced the first aerosol spectrometer capable of detecting coincidence. The model 3321 builds upon this accomplishment with a redesigned nozzle configuration and improved signal processing. These enhancements provide greater small-particle sizing efficiency, improved accuracy of mass-weighted distributions, and virtual elimination of false background counts. Coincidence affects all single-particle counting instruments. It occurs when more than one particle is present in an instrument's measuring volume. This can distort sizing information and lead to underreporting of particle concentration.

The APS™ 3321 uses a patented optical system with two partially overlapping laser beams to detect coincidence. As a particle passes through these overlapping beams, it generates one signal with two crests. The time between the crests provides aerodynamic particle size information. If more than one particle is in the viewing volume, more than two crests appear, and the APS™ spectrometer logs this separately as a coincidence event. While it does not eliminate the occurrence of coincidence, the instrument does effectively limit the effect of coincidence on particle size distributions.

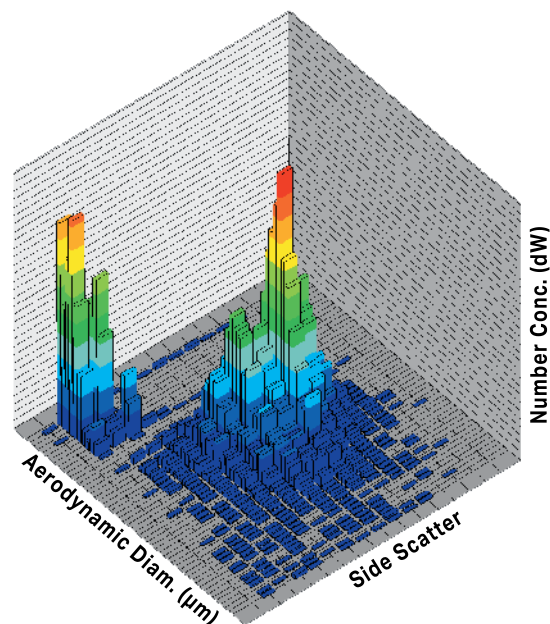

Why Include Light-Scattering Intensity?

Converting light-scattering intensity to geometric size often produces inaccuracies when sizing particles of different shapes and refractive indices. The APS™ spectrometer measures relative light-scattering intensity, but rather than use it to determine particle size, the APS™ spectrometer logs this measurement as a separate parameter. Light-scattering measurements can be made alone, in addition to aerodynamic diameter, or correlated to aerodynamic diameter on a particle-by-particle basis. Thus, researchers are able to gain additional insights into aerosol composition.

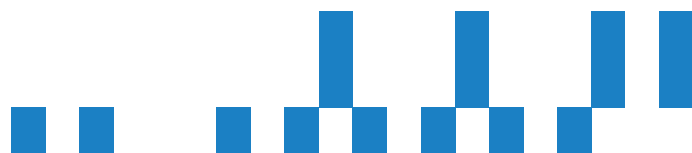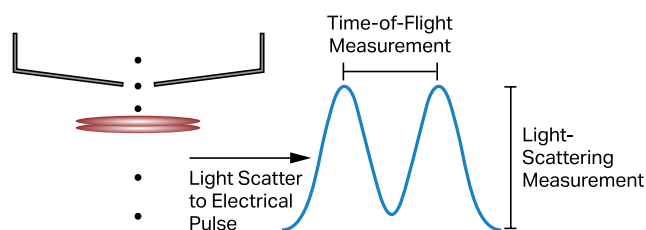

Accessories and Software

Accessories



Dust Aerosol Generator 3410 disperses dry dust and powders for applications that need continuous and stable dosing with high accuracy.



APS™ spectrometer configured with optional Aerosol Diluter 3302A for conditioning high-concentration aerosols.




APS™ spectrometer with optional Impactor Inlet 3306 for MDI/DPI aerosol analysis.


Software

For setup and initial sampling, you can operate the APS™ 3321 without a computer using the front panel control knob and built-in display. However, to save, interpret, or print data, you must use a computer or some other data collection system. The model 3321 includes the Aerosol Instrument Manager® software, designed for use with Windows® operating systems. The Aerosol Instrument Manager software controls instrument operation, plus

it provides impressive file management capabilities and numerous choices for data display. Graphs and tables make it easy to view channel data as well as raw data, giving you the highest resolution possible. You can view all data types—time-of-flight, light-scattering, or correlated data—with the Aerosol Instrument Manager software. An export function allows easy transport of data files to spreadsheet or other applications for customized data handling.

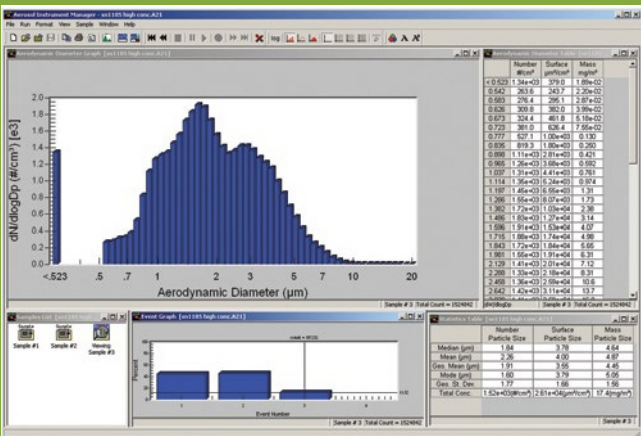

Three graphs showing aerodynamic diameter, side scatter, and correlated data

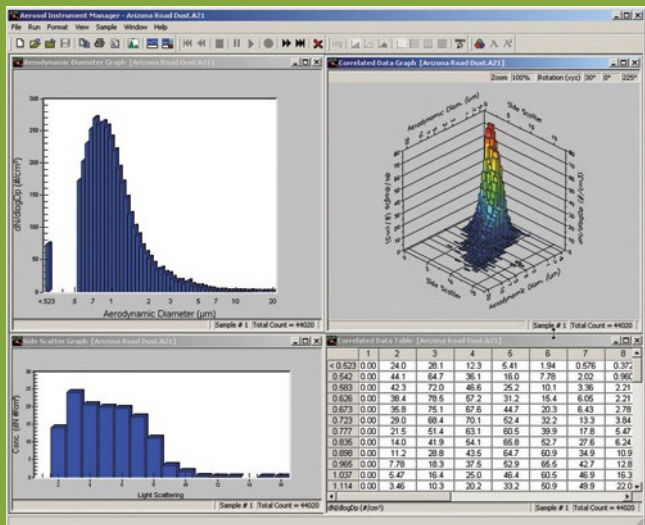

Aerodynamic diameter and events displayed simultaneously



Specifications

Aerodynamic Particle Sizer®

Model 3321

Measurement Technique

Time-of-flight of individual particles measured in an accelerating flow field with a single, high-speed timing processor; coincidence detection achieved using a patented, double-crest optical system; particle size binning based on internally stored calibration curve

Particle Size Range

0.5 to 20 µm aerodynamic sizing, 0.37 to 20 µm optical detection (PSL equivalent)

Aerodynamic Size Resolution

0.02 µm at 1.0 µm, 0.03 µm at 10 µm

Display Resolution

Particle Size	32 channels per decade of particle size (logarithmic), 52 channels total; 1,024 bins of raw time-of-flight data (4 nsec per bin) in uncorrelated mode
---------------	---

Light Scattering (log-compressed)

16 channels of light-scattering intensity (displayed);
64 channels of raw light-scattering data

Particle Type

Airborne solids and nonvolatile liquids

Maximum Recommended Particle Concentration

1,000 particles/cm³ at 0.5 µm with <5% coincidence; 1,000 particles/cm³ at 10.0 µm with <10% coincidence; usable data up to 10,000 particles/cm³

Minimum Particle Concentration

0.001 particle/cm³

Concentration Accuracy

±10% of reading plus variation from counting statistics

Maximum Processing Rate for Aerodynamic Sizing

>200,000 particles/sec

Sampling Time**

Programmable and repeatable from 1 sec to 18 hr per sample; sampling schedules selected by user

Flow Rates*

Aerosol Sample	1.0 L/min ±0.1
Sheath Air	4.0 L/min ±0.1
Total	5.0 L/min ±0.2

Specifications are subject to change without notice. TSI, the TSI logo, Aerodynamic Particle Sizer, and Aerosol Instrument Manager are registered trademarks of TSI Incorporated in the United States and may be protected under other country's trademark registrations. APS is a trademark of TSI Incorporated. Windows is a registered trademark of Microsoft Corporation. Pentium is a registered trademark of Intel Corporation.



MALAYSIA DISTRIBUTOR

ENVIROTERM SDN. BHD.

HEAD OFFICE

Lot 5028, Jalan 18/62,
Taman Perindustrian Sri Serdang,
43300 Seri Kembangan,
Selangor D.E., Malaysia.

T: +603 8210 8338

E: sales@enviroterm.com

W: www.enviroterm.com

NORTHERN OFFICE

5112, Jalan Capri,
Taman Capri,
12100 Butterworth,
Pulau Pinang, Malaysia.

T: +604 331 1371

F: +604 331 1373

E: sales@enviroterm.com

W: www.enviroterm.com

SOUTHERN OFFICE

20-09 Austin 18,
Jalan Austin Perdana 3,
Taman Austin Perdana,
81100 Johor Bahru,
Johor, Malaysia.

T: +607 364 8080

E: sales@enviroterm.com

W: www.enviroterm.com

Atmospheric Pressure Correction

Automatic correction between 400 and 1,030 mbar
(full correction between 700 and 1,030 mbar)

Laser Source

30-mW, 655-nm laser diode

Detector

Avalanche photodetector (APD)

Front-panel Display

320 x 240 pixels

Operating Temperature

10 to 40°C (50 to 104°F)

Operating Humidity

10 to 90% R.H., non-condensing

Power

100 to 240 VAC, 50/60 Hz, 100 W, single phase or 24 VDC

Computer Requirements

Pentium® 4 processor with 2-GHz speed or better, at least 512 MB RAM

Operating System

Windows® 7 operating system or better

Communications

DSUB 9-pin RS-232

Outputs

Digital	I/O 15-pin port (3 inputs, 3 outputs) for external device control and two analog inputs (0 to 10 V)
Configurable Analog	BNC (0 to 10 V)
Analog Pulse	BNC
Digital Time-of-flight	BNC

Dimensions

Aerosol Inlet	3/4 in. (O.D.)
Sensor (HWD) 15 in.)	18 cm x 30 cm x 38 cm (7 in. x 12 in. x 15 in.)
Weight	10 kg (22 lb.)

*Flow accuracy affects size and concentration measurements. Flow specifications are the minimum expected performance of a properly calibrated instrument at standard temperature and pressure.

**Short sampling times are limited by processing overhead, communication delays, and aerosol transport delays. Longer sampling times are recommended for best results.

To Order

Aerodynamic Particle Sizer® Spectrometer

Specify	Description
3321	APS™ sensor with Aerosol Instrument Manager® software

Optional Accessories

Specify	Description
3302A	Aerosol Diluter
3306	Impactor Inlet
3410	Dust Aerosol Generator
390069	Data Merge Software Module